



## Duty Station DS-110



**Description:** Cornell DS-110 Duty Station offers immediate Annunciation of any call on the system via tone and red LED on a single status 4000 system.

**Operation:** The DS-110 Duty Station has a manual high or low volume tone switch that is provided for an audible alert to staff. Steady red LED indication with pulsing tone.

**Mounting:** The satin finish stainless steel faceplate with silk-screened designations may be flush mounted on a standard outlet box with single-gang plaster ring, or surface mounted on a Wiremold 5748 or equivalent. Field wiring terminations are pigtailed.



**Engineering Specifications:** The duty station shall be CORNELL Model DS-110. Incoming emergency calls shall be indicated by a (steady) red LED indicator and pulsing tone. The station shall have a manual switch for High-Low volume. The station shall fit on a standard single gang plaster ring or Wiremold 5748 surface box or equal. Minimum depth shall be 1 3/4". Visual indicators shall be LED's. Incandescent lamps not accepted. Terminations for field wiring shall be pigtailed.

### Technical Information:

- Power Requirements: 24VDC
- Operating Environment: 50-120°F Indoor Non-condensing
- Physical Faceplate Dimensions: 4 1/2 "H x 2 3/4 "W (1 Gang)
- Mounting: Single-Gang back box with 1 3/4" minimum depth
- Wiring: Terminations are Pigtailed



Available in 1-6 gang sizes:

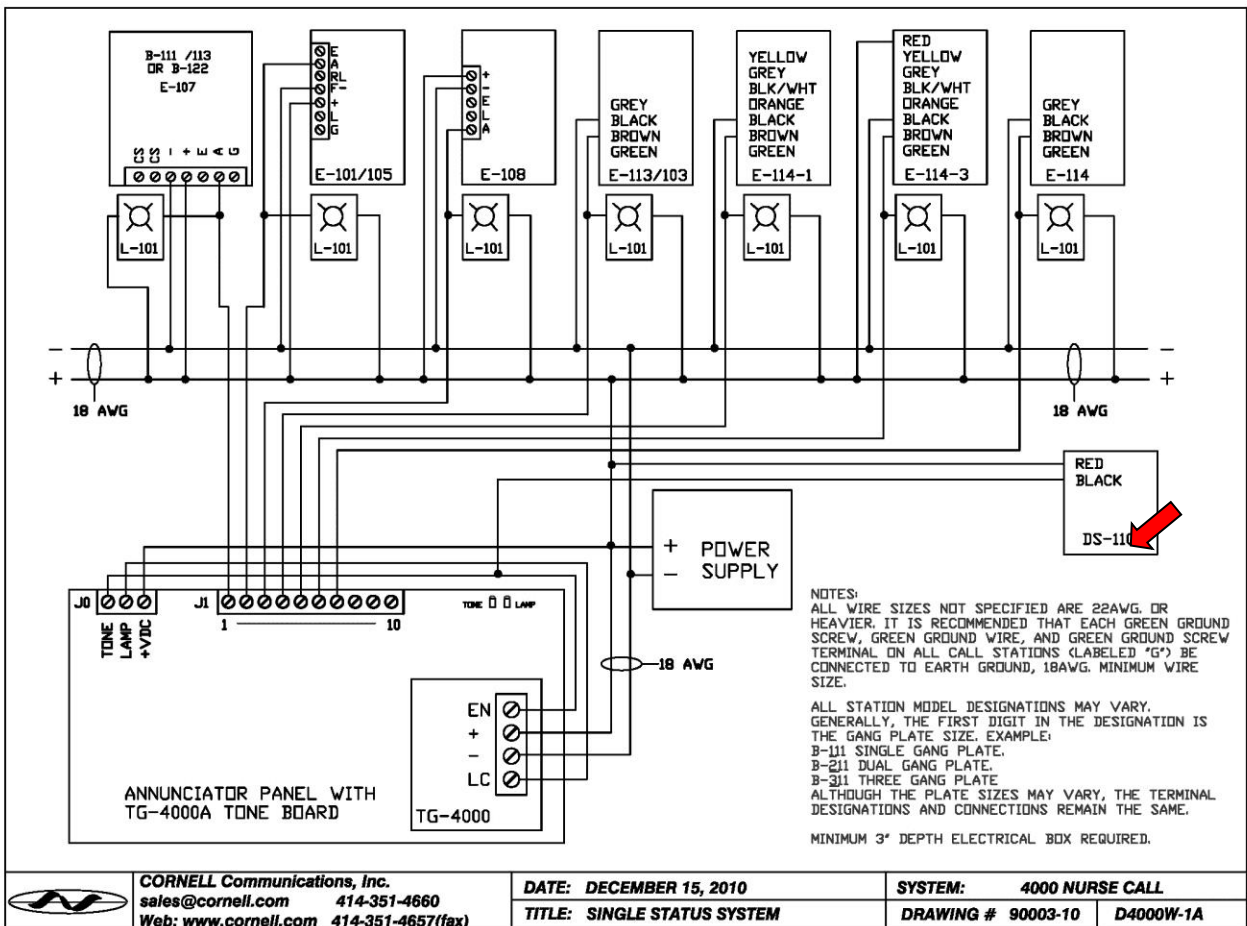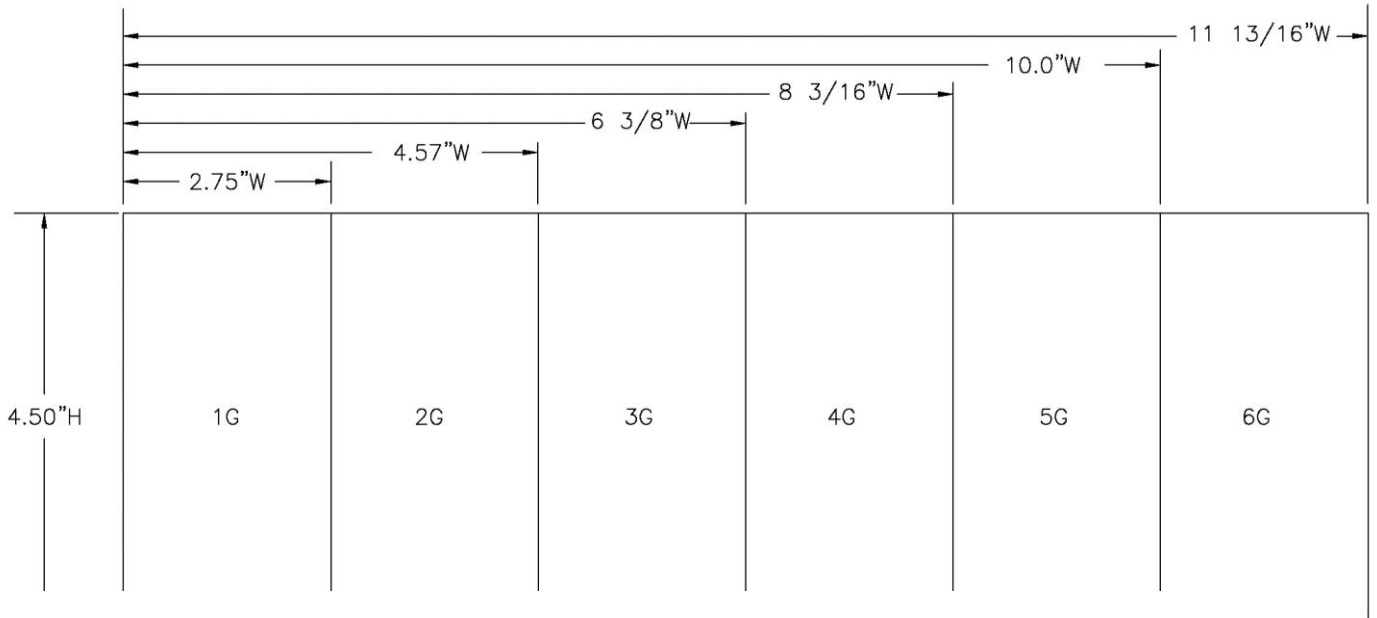

|  |  |  |   |           |
|--|--|--|---|-----------|
|  | CORNELL Communications, Inc.<br>sales@cornell.com 414-351-4660<br>Web: www.cornell.com 414-351-4657(fax) | DATE: DECEMBER 15, 2010<br>TITLE: SINGLE STATUS SYSTEM | SYSTEM: 4000 NURSE CALL<br>DRAWING # 90003-10 | D4000W-1A |
|  |  |  |   |           |

CORNELL COMMUNICATIONS, INC.

Milwaukee, Wisconsin USA • 800-558-8957 • 414-351-4660 • Fax 414-351-4657  
 www.cornell.com • sales@cornell.com

